


Water flow meter/totalizer shall be connected post filter. Meter Sterility cannot be guaranteed. Please note flow direction on filter housing (IN and OUT). Following Filtration, do not drain water from filter. Disconnect filter and place caps on ends while avoiding water loss. If sampling chlorinated waters, use injector containing sodium thiosulfate to ensure chlorine residual neutralization. Following filtration, add Sodium Thiosulfate crystals to inlet side of filter housing and seal with cap.

Effluents containing low chlorine residuals (<0.5ppm) may be dechlorinated following sample collection by addition of thiosulfate to filter housing)

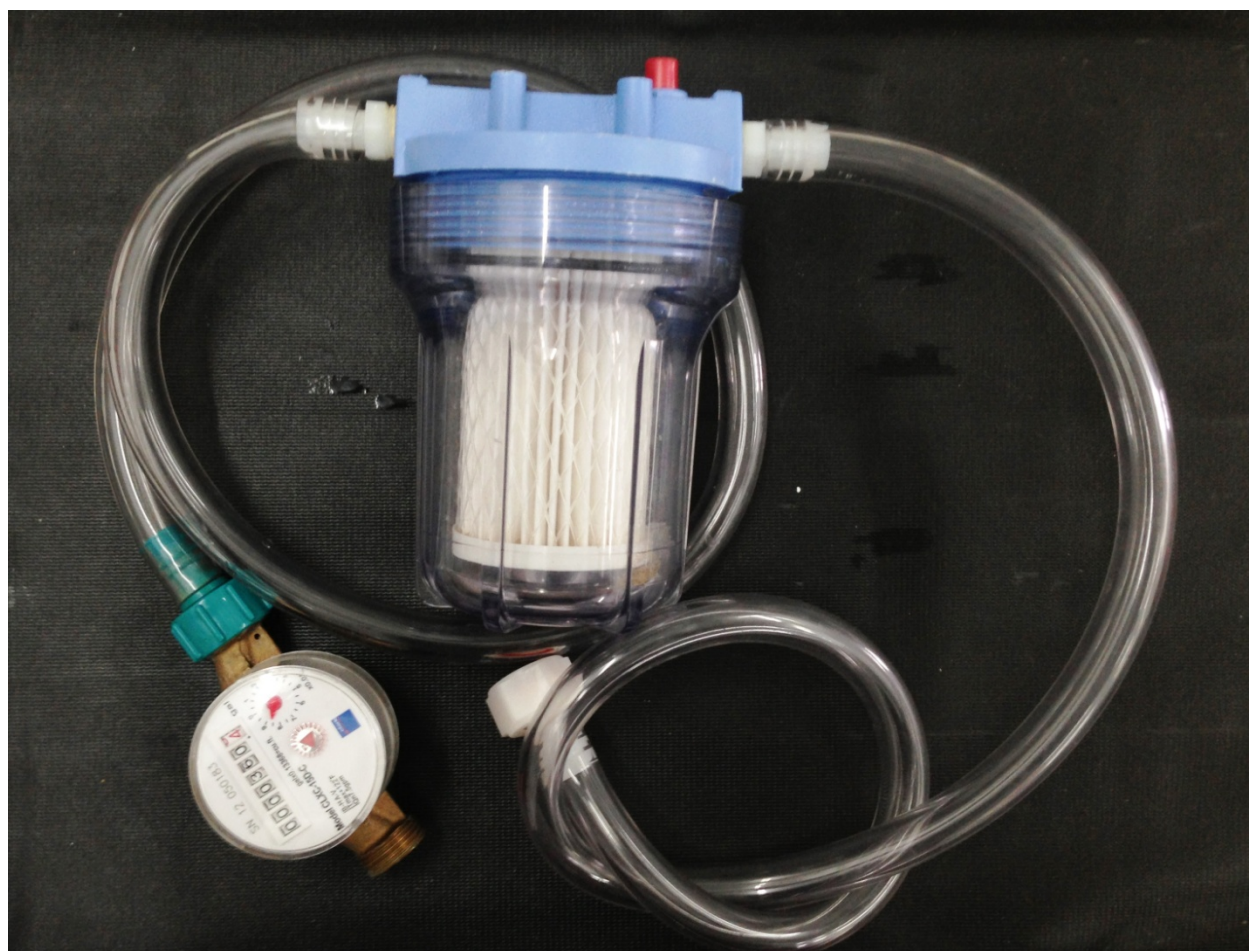

Recommended Flow Rate 1.0 gallon/minute
Flow rate shall not exceed 2.0 gallons/ minute